



Liquid Handling Station

PRODUCT
INFORMATION

BRAND Liquid Handling Station

Automating an ELISA assay for the characterization of antibody functionality

Introduction

Jackson ImmunoResearch saw a need to monitor antibody performance at sequential stages of production. Antibody characterization was previously done using a time consuming, complex and physically demanding method which constrained testing to the final step in the process. This led to the loss of valuable decision making opportunities along the way which could improve product quality and efficiencies in manufacture. To solve this problem, Jackson ImmunoResearch's Quality Assurance department developed an automated assay using the BRAND Liquid Handling Station.

Currently, the Quality Assurance department runs about 10-15 samples per week utilizing this new assay. This workload is added on to the requirements of an already busy group. The hope is that this test becomes integrated into the production process. This could potentially double the frequency of testing.

Jackson ImmunoResearch wanted to take pressure off technicians by automating this testing procedure. The expectation

is to ensure precise results that are repeatable and consistent. Using a robot reduces the opportunity for human error. It also frees up technicians to be able to get other work done while the robot is working. Repetitive motion tasks are reduced for a technician as well.

As a first step, an inexpensive liquid handler was purchased to prove that automating this procedure was achievable and would be beneficial. The operation of the robot required a QA technician to learn computer coding in order to develop and execute protocols within the operation software. The robot's software was not intuitive and writing each program was very tedious. After working with the robot for almost a year, it never functioned correctly due to manufacturing and design issues. However, it did function well enough to provide successful proof of concept testing. Jackson ImmunoResearch then decided to look for a system that was easy to use, reliable, and affordable. The BRAND Liquid Handling Station (LHS) seemed promising. Following a successful demo of the LHS, the instrument was purchased and put right to work.

Material and method



Figure 1
Liquid Handling Station using the 20-300 µl 8-channel Liquid End.

The LHS was used to prepare ELISA plates, while in parallel ELISA plates were also prepared by a technician for comparison of results. In this application, the LHS coated ELISA plates with 100 µl/well by multi-dispense pipetting pre-diluted coating solutions from 2 ml microcentrifuge tubes using the 1 ml single channel Liquid End (LE). The robot was able to dispense 10 wells with 1 aspiration. Conversely, a technician coated ELISA plates using a manual hand-held 50-300 µl multichannel pipette.

The LHS added 300 µl/well blocking solution to all wells from a 6-well reservoir using the 20-300 µl 8-channel LE. The technician, again, used a manual hand-held 50-300 µl multichannel pipette to block plates. After another incubation period, the LHS performed serial dilutions in a deep-well plate and loaded the ELISA plates using the 20-300 µl 8-channel LE. The initial dilutions were done by the technician with a pre-loaded dilution plate added to the LHS deck.

The LHS added diluent and serially diluted, then added 100 µl/well to the ELISA plates in duplicate wells. This same process was performed by the technician by hand. The next step entailed adding 100 µl/well diluted detection antibody to all wells from a 6-well reservoir, similar to the blocking step, using the 20-300 µl 8-channel LE. The final step of the assay that the LHS accomplished was adding 100 µl/well substrate to all wells. Once more, this used the 20-300 µl 8-channel LE pipetting from a 6-well reservoir into the ELISA plate. The technician completed these two tasks by hand using a manual multichannel pipette. All washing steps and plate reading were performed outside of the LHS.

Benefits of using the LHS

Programming this robot is incredibly intuitive. This benefits bench scientists who usually don't have a formal education in computer coding. To be able to drag and drop onto a virtual deck that looks just like the real thing and adjust all aspects of set-up easily makes programming stress free.

After the program is written, checking the efficiency and accuracy of the new protocol can be done with the simulate feature. This allows the user to catch mistakes before utilizing samples and consumables on an errant program. One of the most helpful features incorporated into the dilution program was being able to add a pause into the protocol. The pause was added with an instruction to wash and add the ELISA plate to the appropriate deck position. This way, the ELISA plate did not sit on the deck dry after being washed, waiting for the robot to dilute the samples.



Figure 2
The virtual deck of the software of the Liquid Handling Station looks like the real worktable.

Results summary

The LHS performed the ELISA very similarly to a technician. Below shows a summary of the results and compares the two methods.

Sample	QA Technician	BRAND LHS	Difference
protein #1	0.30	0.32	-0.02
protein #2	0.11	0.11	0.00
protein #3	0.04	0.05	-0.01
protein #4	0.77	0.77	0.00
protein #5	0.05	0.06	-0.01

Table 1
Test Sample #1

Sample	QA Technician	BRAND LHS	Difference
protein #1	0.16	0.17	-0.01
protein #2	0.02	0.02	0.00
protein #3	0.07	0.07	0.00
protein #4	0.25	0.28	-0.03
protein #5	0.02	0.02	0.00
protein #6	0.24	0.26	-0.02
protein #7	0.23	0.21	0.02
protein #8	0.06	0.07	-0.01

Table 2
Test Sample #2


Sample	QA Technician	BRAND LHS	Difference
protein #1	1.46	1.42	0.04
protein #2	14.21	14.29	-0.08
protein #3	8.40	8.44	-0.04

Table 3
Test Sample #3

Sample	QA Technician	BRAND LHS	Difference
protein #1	0.34	0.37	-0.03
protein #2	0.15	0.16	-0.01
protein #3	0.00	0.00	0.00
protein #4	0.05	0.05	0.00
protein #5	0.18	0.19	-0.01

Table 4
Test Sample #4

Target protein curves plotted from the QA Technician's data and the LHS's data also look very similar

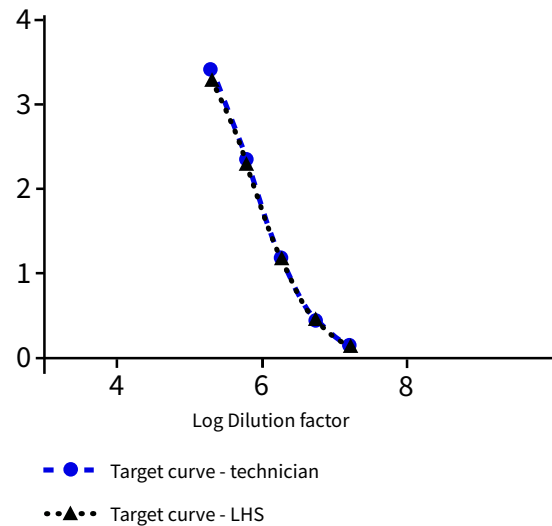

As is evident with the data analyses, these two curves and the ODs from the samples relate to each other in the same way regardless of whether a person is running the test or the LHS is doing the pipetting.

Summary

For Jackson ImmunoResearch, integrating the BRAND Liquid Handling Station into the testing repertoire seemed like a logical next step to continually improve testing methods and optimize production. This particular robot allows

for intuitive programming and accurate pipetting. These features help free up time for a technician to be able to complete a task while the LHS easily performs another.

BRAND GMBH + CO KG

P.O. Box 1155 | 97861 Wertheim | Germany

T +49 9342 808 0 | F +49 9342 808 98000 | info@brand.de | www.brand.de



BRAND. For lab. For life.®

BRAND®, BRAND. For lab. For life.®, as well as the BRAND figurative mark are registered trademarks or trademarks of BRAND GMBH + CO KG, Germany. The BRANDGROUP figurative mark is registered trademark or trademark of Brand Group SE & Co. KG, Germany. All other trademarks mentioned or depicted here are the property of the respective owners.

Our technical literature is intended to inform and advise our customers. However, the validity of general empirical values, and of results obtained under test conditions, for specific applications depends on many factors beyond our control. Please appreciate, therefore, that no claims can be derived from our advice. The user is responsible for checking the appropriateness of the product for any particular application.

California Residents: For more information concerning California Proposition 65, please refer to www.brand.de/calprop65.

Subject to technical modification without notice. Errors excepted.



Find accessories and replacement parts, user manuals, test instructions (SOP) and product videos at shop.brand.de



Further information on products and applications can be found on our YouTube channel: [mylabBRAND](#)

© 2021 BRAND GMBH + CO KG | Printed in Germany | 0524

BRAND (Shanghai) Trading Co., Ltd.
Shanghai, China

Tel.: +86 21 6422 2318
info@brand.com.cn
china.brand.com.cn

BRAND Scientific Equipment Pvt. Ltd.
Mumbai, India

Tel.: +91 22 42957790
customersupport@brand.co.in
www.brand.co.in

BRANDTECH® Scientific, Inc.
Essex, CT. United States of America

Tel.: +1 860 767 2562
info@brandtech.com
www.brandtech.com